


PROJECT RESULTS: Tracer Gas Airflow Measurement System

Accuracy Verification

Laboratory testing of Tracer Gas system versus narrow-band nozzle box

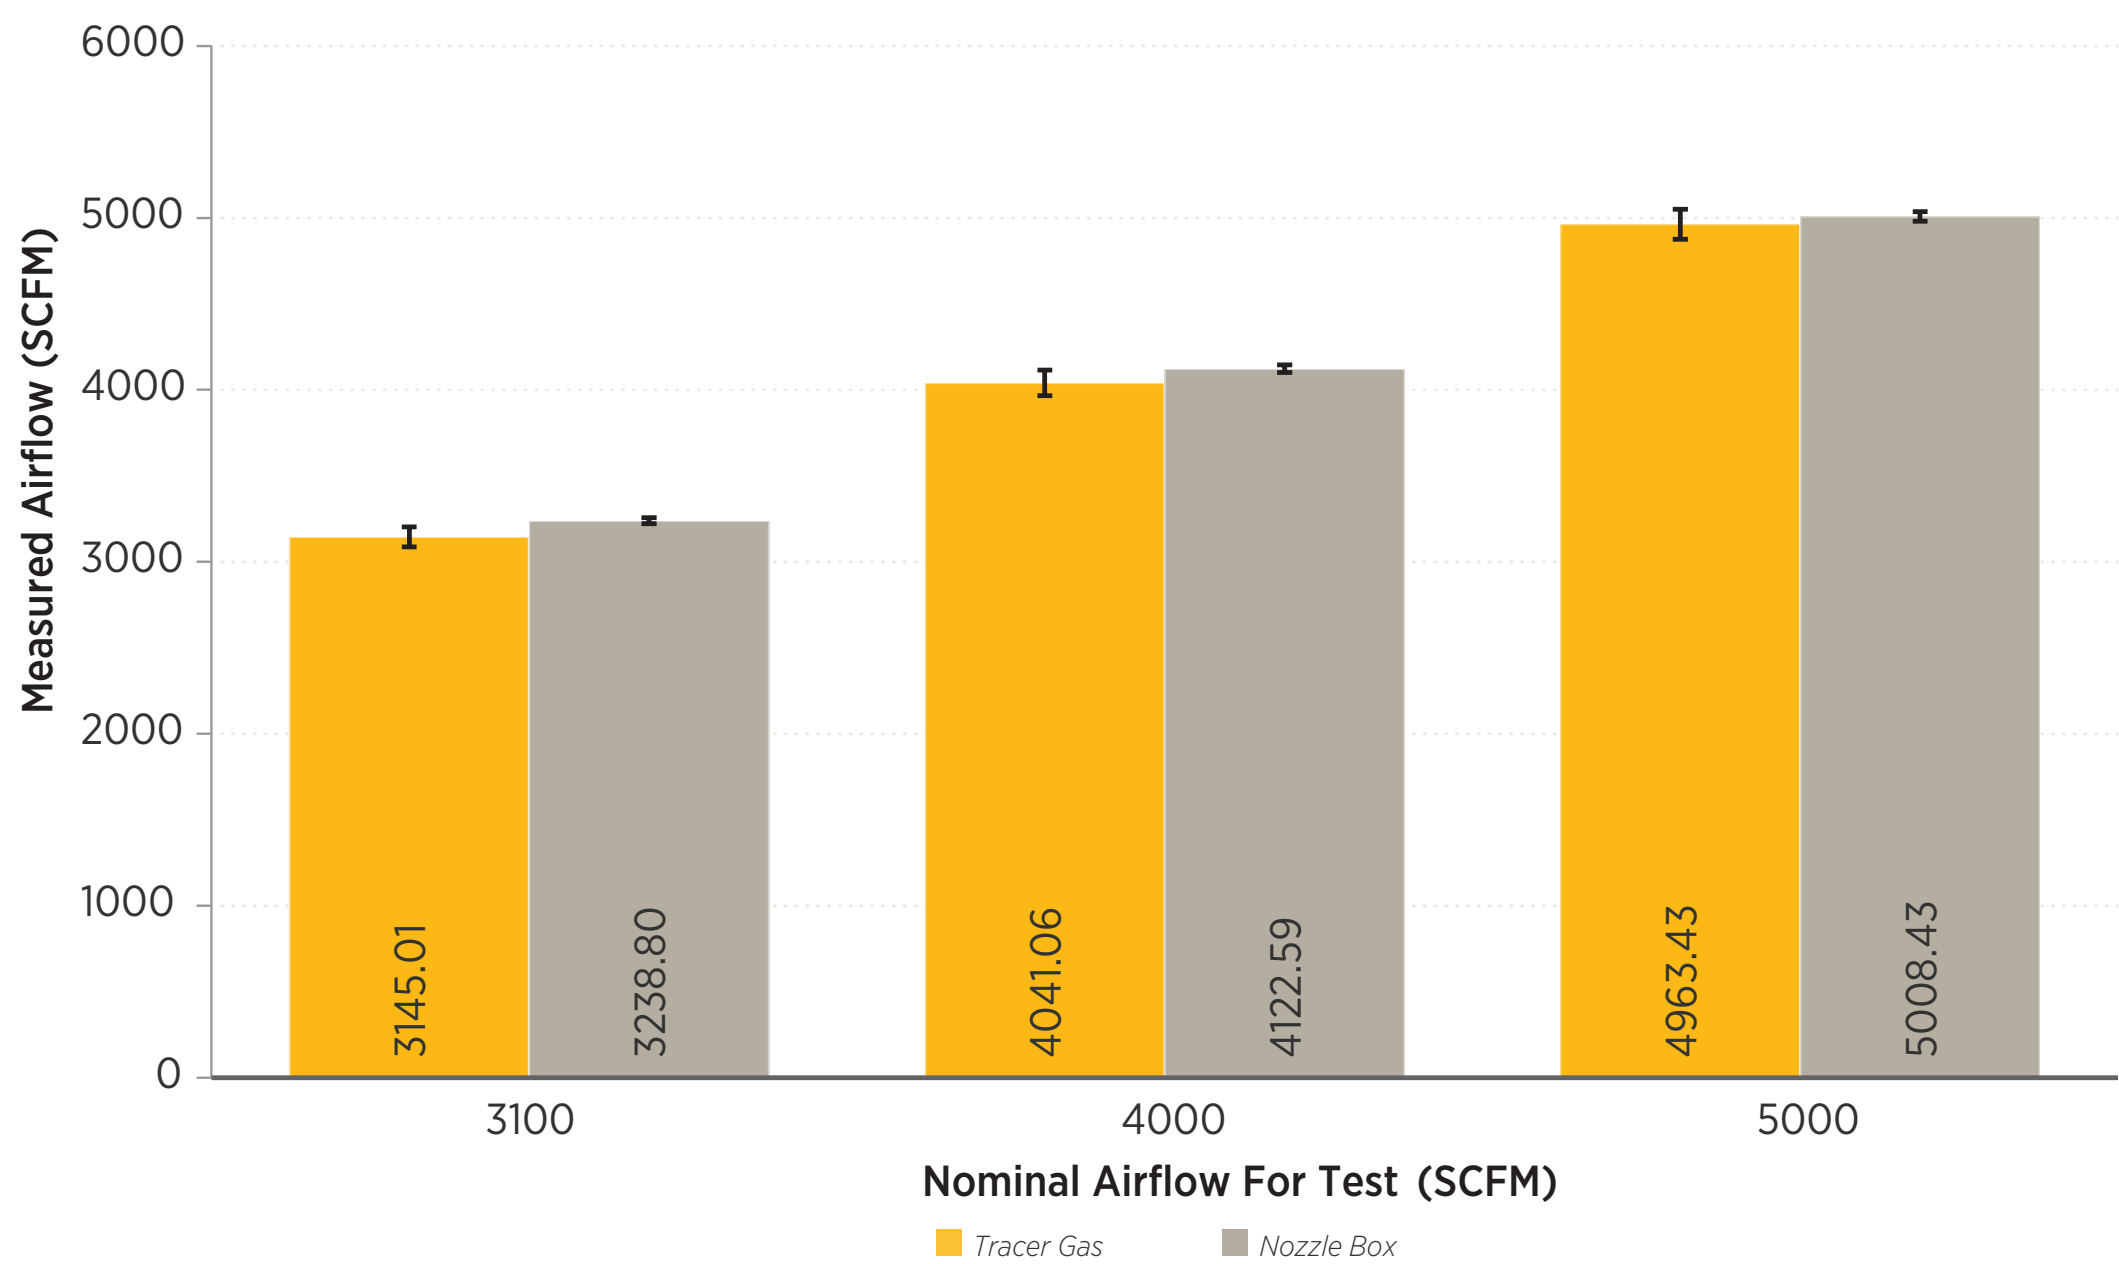

Measurement Range

Wide ranging airflow measurement accuracy

